

Batch Verification

KLOW 80 MG

Independent laboratory documentation

LABORATORY

Janoshik

TESTING PERIOD

24 Jun - 07 Jul 2026

Original reports and raw data reproduced in full.

Verification summary

A consolidated overview of the attached independent laboratory reports. Original Janoshik documents and supporting raw data follow unchanged.

PRODUCT

KLOW 80 mg

BATCH

KL802607

LAB

Janoshik

MEASURED COMPOSITION

Task #195435 / 29 Jun 2026

GHK-CU (GHK CONTENT / COPPER)

53.62 mg (46.87 mg / 6.75 mg)

TB-500 (TB4)

11.21 mg

BPC-157

11.77 mg

KPV

11.75 mg

ENDOTOXIN

53.799 EU/vial

Task #195436 / 24 Jun 2026

MICROBIAL TESTING

TAMC PASS / TYMC PASS

Task #195438 / 07 Jul 2026

HEAVY METALS

As, Cd, Hg and Pb: not detected

Task #195439 / 29 Jun 2026

DOCUMENT ORDER

- 1 Composition report and chromatogram
- 2 Endotoxin report
- 3 Microbial testing report

- 4 Heavy-metals report
- 5 Heavy-metals raw data and spectra

Summary prepared by OPTide from the attached laboratory reports. Results apply only to the submitted sample identified as KL802607. No information on this page replaces the original laboratory documentation.

TEST REPORT



E-mail: info@janoshik.com
Web: www.janoshik.com

Task Number #195435

Testing ordered > 14 JUN '26

Sample received > 16 JUN '26

Client OPTide

Sample KLOW

Manufacturer OPTide

Batch KL802607

Sample description >

See picture or pictures attached.

Tests requested >

KLOW (GHK or GHK-Cu/ TB-500/ BPC-157/ KPV) analysis

Results >



GHK-Cu (GHK content) [Copper Content]	53.62 mg (46.87 mg) [6.75 mg]
TB-500 (TB4)	11.21 mg
BPC-157	11.77 mg

Comments >

KPV: 11.75 mg

Analysis conducted > 29 JUN 2026

Signature >

A handwritten signature in black ink, appearing to be 'Janoshik' or similar, located to the right of the 'Signature >' label.

Verify this test at www.janoshik.com/verify/ with the following unique key

I72ILH6TGSEU



SHIMADZU

LabSolutions

Analysis Report


<Sample Information>

Sample Name : 23929-2 KLOW 80mg endo+norm.test+HM
 Sample ID : 016
 Data Filename : 23929-2 KLOW 80mg endo+norm.test+HM_019.lcd
 Method Filename : 251007_MeOH-H2O-TFA_peptidy2_Blend_0.5_+780nm Cu.lcm
 Batch Filename : 20260625_2.lcb
 Vial # : 3-29
 Injection Volume : 0.5 uL
 Date Acquired : 26.06.2026 3:28:33
 Date Processed : 29.06.2026 12:46:46

Sample Type : Unknown
 Acquired by : System Administrator
 Processed by : System Administrator

<Chromatogram>

mAU

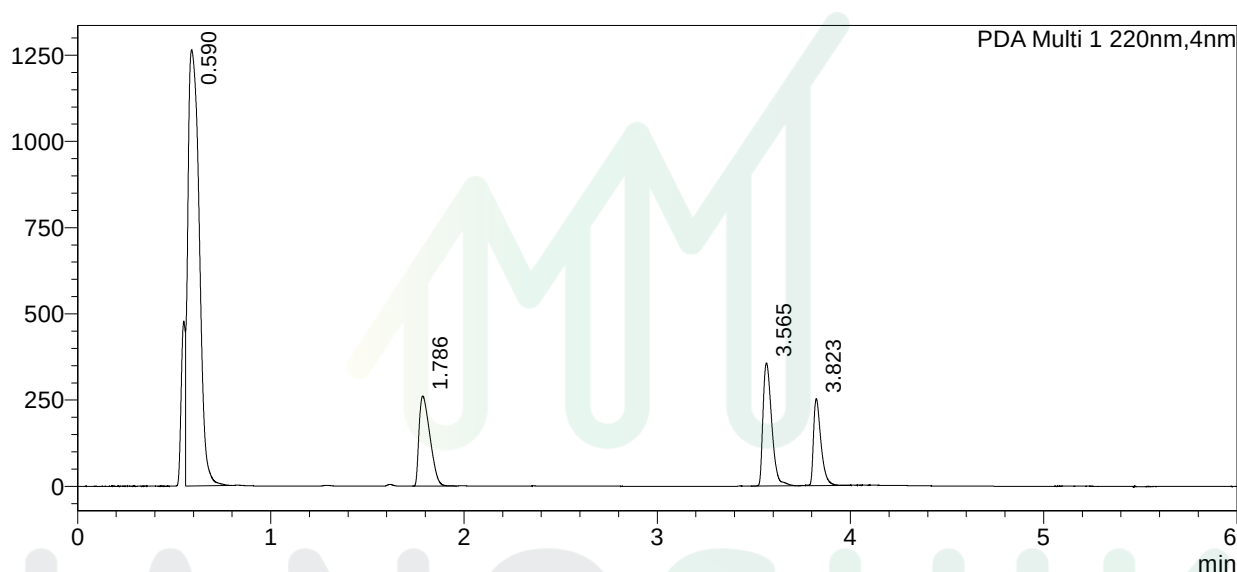

<Peak Table>

PDA Ch1 220nm

Peak#	Ret. Time	Area	Conc.	Unit	Name	Area%
1	0.590	5212612	0.00			64.880
2	1.786	1021669	11.75	mg	KPV	12.716
3	3.565	1123639	11.77	mg	BPC-157	13.986
4	3.823	676357	11.21	mg	TB-500 (TB4)	8.418
Total		8034277				100.000

TEST REPORT



E-mail: info@janoshik.com
Web: www.janoshik.com

Task Number #195436

Testing ordered > 14 JUN '26

Sample received > 16 JUN '26

Client OPTide

Sample KLOW

Manufacturer OPTide

Batch KL802607

Sample description >

See picture or pictures attached.

Tests requested >

Endotoxin Analysis

Results >



Endotoxin	53.799 EU/Vial.

Comments >

Analysis conducted > 24 JUN 2026

Signature >



Verify this test at www.janoshik.com/verify/ with the following unique key

FRYSMGPJEJRH

TEST REPORT



E-mail: info@janoshik.com
Web: www.janoshik.com

Task Number #195438

Testing ordered > 14 JUN '26

Sample received > 16 JUN '26

Client OPTide

Sample KLOW

Manufacturer OPTide

Batch KL802607

Sample description >

See picture or pictures attached.

Tests requested >

Sterility Testing

Results >



TAMC	PASS
TYMC	PASS

Comments >

Analysis conducted > 07 JUL 2026

Signature >



Verify this test at www.janoshik.com/verify/ with the following unique key

CTCH4FJ77SR7

TEST REPORT



E-mail: info@janoshik.com
Web: www.janoshik.com

Task Number #195439

Testing ordered > 14 JUN '26

Sample received > 16 JUN '26

Client OPTide

Sample KLOW

Manufacturer OPTide

Batch KL802607

Sample description >

See picture or pictures attached.

Tests requested >

Heavy Metals Analysis

Results >



As	not detected.
Cd	not detected.
Pb	not detected.

Comments >

Hg: not detected. Although the raw data show low ppm values for heavy metals, these do not necessarily indicate true detection. As shown in the attached graphs, the signals are consistent with electronic noise inherent to the detection system; therefore, the results were concluded as "not detected".

Analysis conducted > 29 JUN 2026

Signature >



Verify this test at www.janoshik.com/verify/ with the following unique key

8NGZCINBMRLQ

Sample : 23929-2
 Operator: MB
 Comment : Comment
 Group : Hg_Pb_Cd
 Date : 2026-06-26 12:52:30

Measurement Condition

Instrument: EDX-7000 Atmosphere: Air Collimator: 10(mm) Sample Cup: Polypropylene

Analyte	TG kV	uA	FI	Acq. (keV)	Anal. (keV)	Time(sec)	DT(%)
Cd	Rh 50	640-Auto	#5	0 - 40	22.72-23.52	Live- 75	30
Hg	Rh 50	640-Auto	#5	0 - 40	9.74-10.24	Live- 75	30
Pb	Rh 50	640-Auto	#5	0 - 40	12.38-12.88	Live- 75	30

Qualitative Result

Element: Cd, Hg, Pb

Peak List

Channel	Line	keV	Net Int. (cps/uA)
Cd	CdKa	23.12	0.0023 Q
Hg	HgLa	9.98	0.0001 Q
Pb	PbLb1	12.62	0.0000 Q

Quantitative Result

Analyte	Result	[3-sigma]	Proc.-Calc.	Line	Int. (cps/uA)
Cd	4.8 ppm	L [2.8]	Quan-EC	CdKa	0.0023
Hg	0.2 ppm	L [1.0]	Quan-EC	HgLa	0.0001
Pb	2.8 ppm	L [3.6]	Quan-EC	PbLb1	0.0000

JANOSHNIK


Sample : 23929-2
Operator: MB

Group : Hg_Pb_Cd
Comment : Comment


Date : 2026-06-26 12:52:30
01/01




[cps/uA] Cd

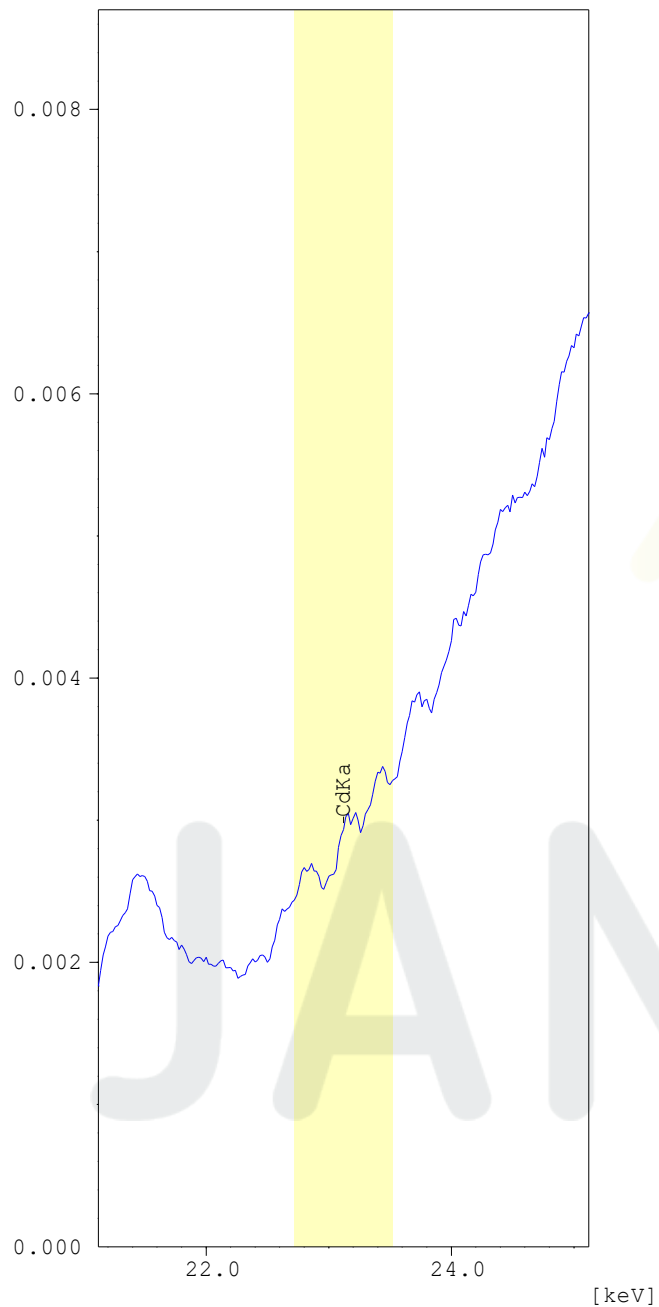

[cps/uA] Hg

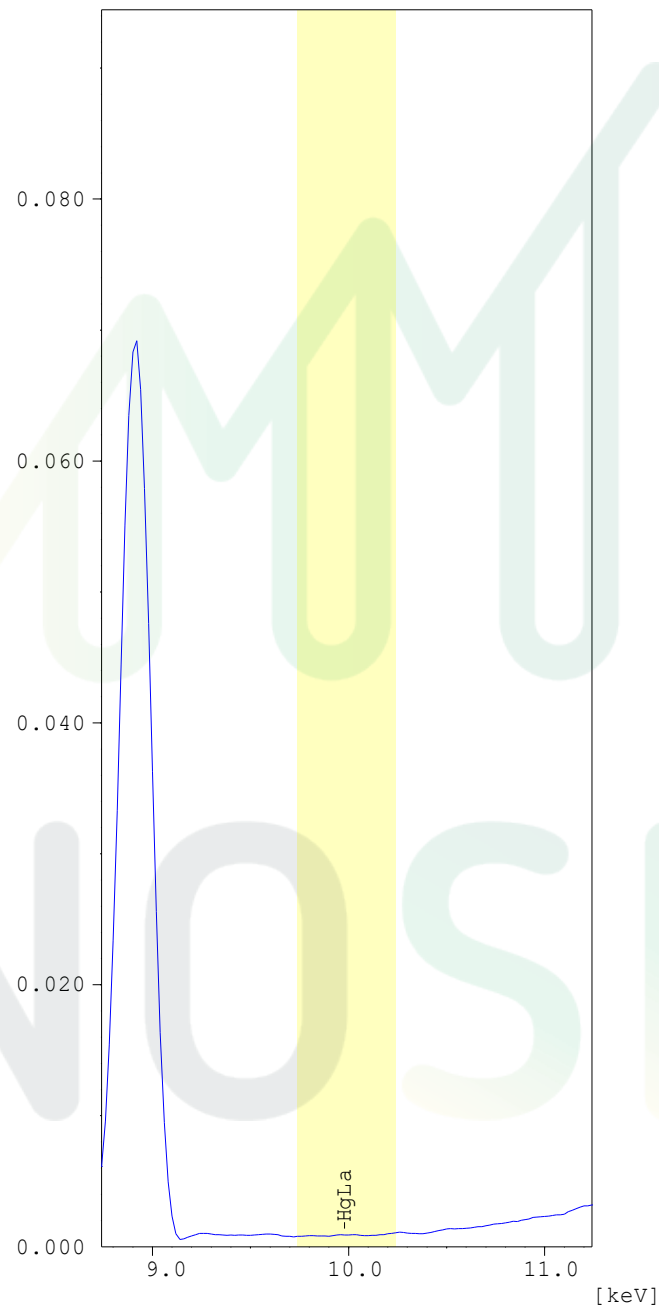

[cps/uA] Pb

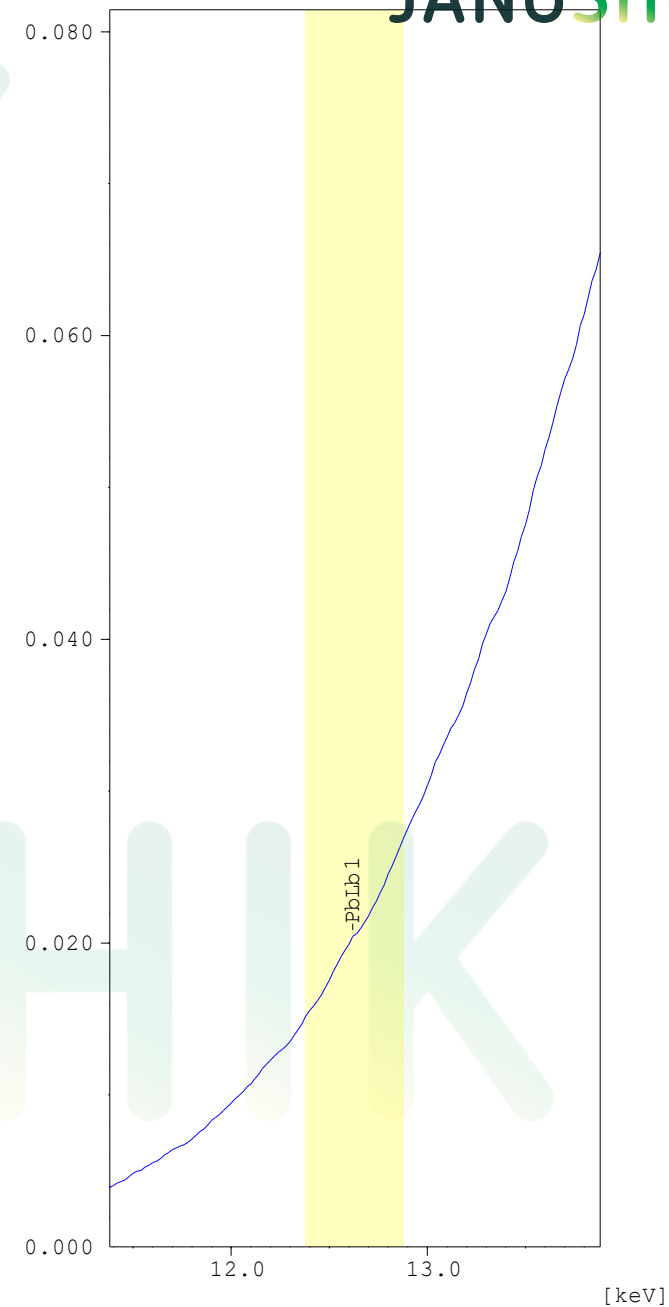


Sample : 23929-2
Operator: MB
Comment : Comment
Group : As_test
Date : 2026-06-26 13:18:08

Measurement Condition

Instrument: EDX-7000		Atmosphere: Air		Collimator: 10 (mm)		Sample Cup: Polypropylene			

Analyte	TG kV	uA	FI	Acq. (keV)	Anal. (keV)	Time (sec)		DT (%)	

As	Rh 50	17-Auto	----	0 - 40	10.30-10.80	Live-	50	30	

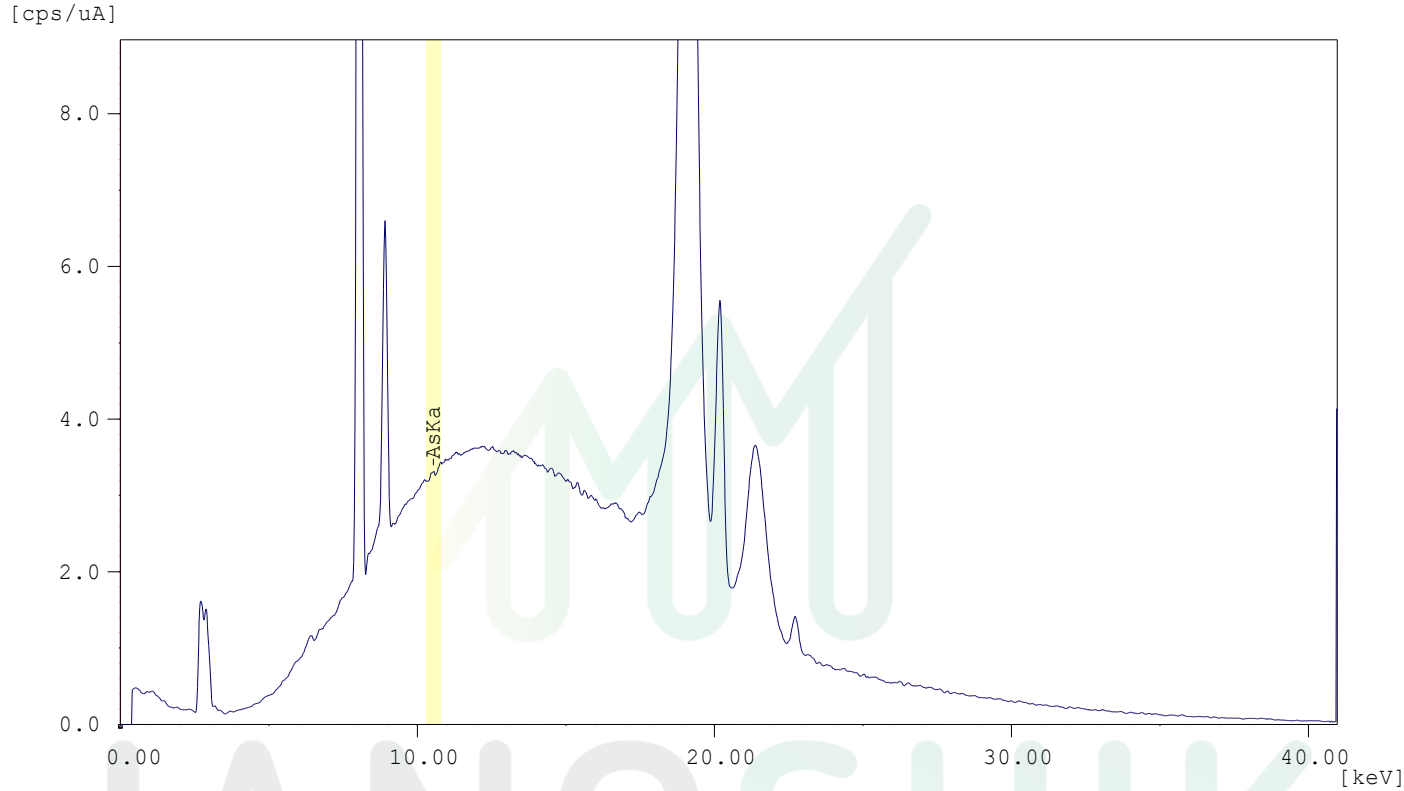

Peak List

Channel	Line	keV	Net Int. (cps/uA)

As	AsKa	10.54	0.0888 Q

Quantitative Result

Analyte	Result	[3-sigma]	Proc.-Calc.	Line	Int. (cps/uA)
As	0.4 ppm	L [4.0]	Quan-EC	AsKa	0.0888