

TEST REPORT



E-mail: info@janoshik.com
Web: www.janoshik.com

Task Number #195445

Testing ordered > 14 JUN '26

Sample received > 16 JUN '26

Client OPTide

Sample Retatrutide

Manufacturer OPTide

Batch RT102607

Sample description >

See picture or pictures attached.

Tests requested >

Common GLP-1 peptide blind test (Semaglutide, Tirzepatide and Retatrutide)

Results >



Retatrutide	11.82 mg
Purity	99.792%

Comments >

Analysis conducted > 30 JUN 2026

Signature >

A handwritten signature in black ink, appearing to be 'Janoshik' or similar, located next to the 'Signature >' label.

Verify this test at www.janoshik.com/verify/ with the following unique key

BV4YPYIWBWJA




Analysis Report

<Sample Information>

Sample Name	: 23929-4 Reta 10mg endo+norm.test+HM		
Sample ID	: 109		
Data Filename	: 23929-4 Reta 10mg endo+norm.test+HM_088.lcd		
Method Filename	: C18- GLP1.lcm		
Batch Filename	: 25_06_2026_01.lcb		
Vial #	: 2-10	Sample Type	: Unknown
Injection Volume	: 0.5 uL		
Date Acquired	: 6/26/2026 3:12:04 AM	Acquired by	: System Administrator
Date Processed	: 6/29/2026 1:07:23 PM	Processed by	: System Administrator

<Chromatogram>

mAU

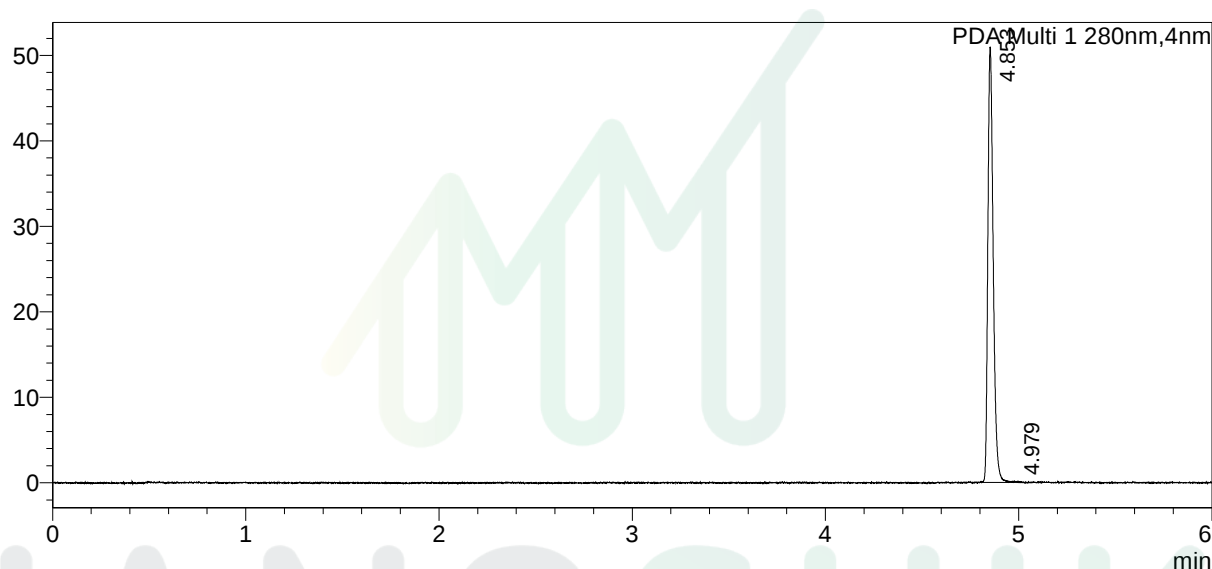

<Peak Table>

PDA Ch1 280nm

Peak#	Ret. Time	Area	Conc.	Unit	Name	Area%
1	4.853	97862	11.82	mg	Retatrutide	99.792
2	4.979	204	0.00			0.208
Total		98066				100.000